




Preparation for use: NONELENS and NONEFRAME

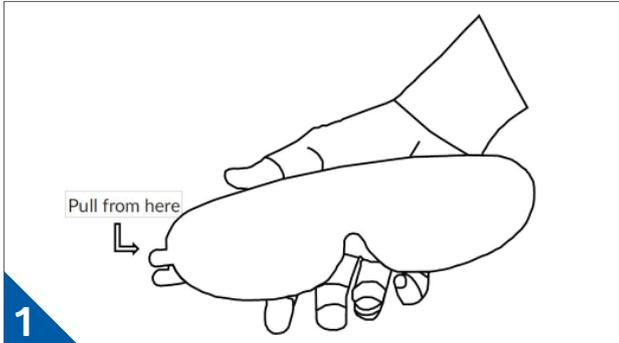


1 Remove the lens (NONELENS) from the dispenser.

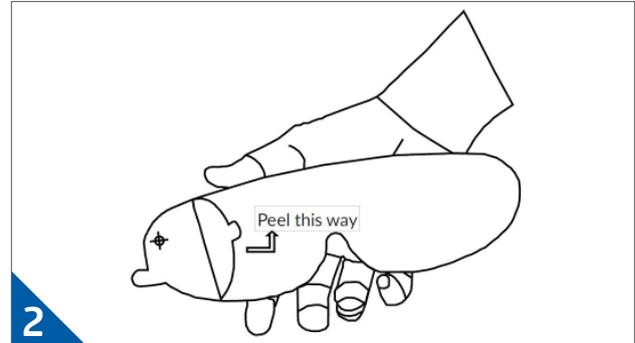


2 Peel away the protective inner film by pulling the upper tab towards you.

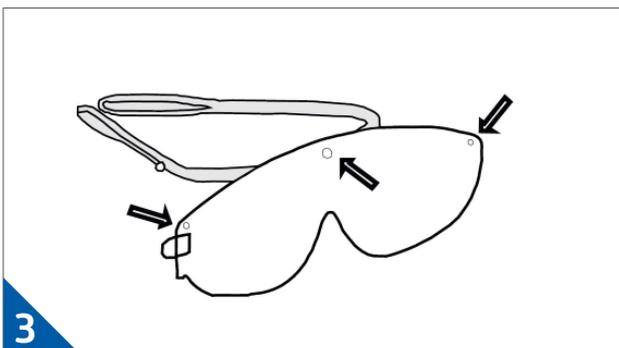

3 Clip three holes into the corresponding reusable frame (NONEFRAME). The remaining film should be on the outside.

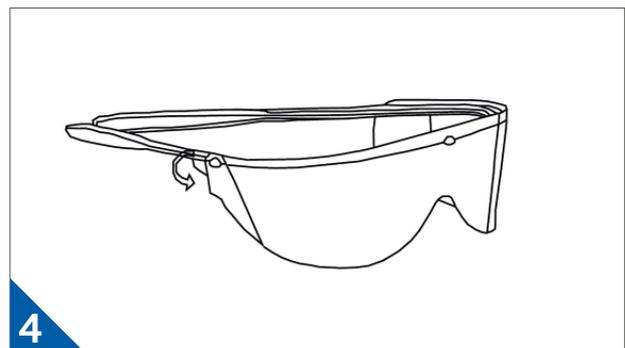

4 Remove the outer peel using the same method in Step 2.

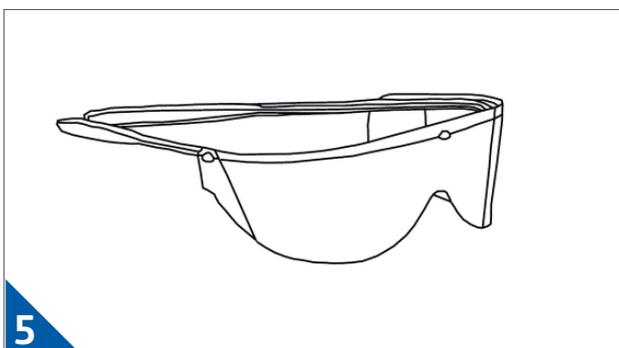

Your device can now be worn and is free from scratches.

Note: To clean or disinfect your NONEFRAME, wipe it gently using liquid with up to 70% Isopropanol.

To learn more about procedure masks, contact your Medline account manager or visit uk.medline.eu